

# RHK Technology

## Application Note

### Integration of the RHK R9*plus* Controller to a Homebuilt Tip-Enhanced Photoluminescence Atomic Force Microscope

Molly A. May,<sup>1</sup> Tao Jiang,<sup>1</sup> Fabian Menges,<sup>1</sup>  
Natalie A. Wasio,<sup>2</sup> and Markus B. Raschke<sup>1</sup>

<sup>1</sup>*Department of Physics, University of Colorado Boulder*

<sup>2</sup>*RHK Technology, Inc.*

#### Introduction

The research in our group is centered around the development and unique applications of nano-optical spectroscopies that enable both nanometer spatial and femtosecond temporal resolution. Recently, we have made significant progress in addressing outstanding questions around excitonic properties in semiconducting 2D materials with tip-enhanced photoluminescence (TEPL) using RHK's R9*plus* controller. For example, here we take advantage of the nano-antenna tip sensitivity to the out-of-plane transition dipole moments of dark excitons to induce, switch, and programmatically modulate the dark exciton emission at room temperature in WSe<sub>2</sub>. With all previous approaches relying on cryogenic temperatures, this approach provides a new and facile way to probe and harness excitonic properties in low-dimensional semiconductors for quantum optoelectronics and other applications.



## Connection to R9plus

The RHK R9plus controller is used to control a custom-built tip-enhanced Raman (TERS) and tip-enhanced photoluminescence (TEPL) atomic force microscope (AFM) system. A schematic is shown in Figure 1. The high voltage outputs of the R9plus control the AFM positioning stage (PI NanoCube P-611.30) and shear force feedback is maintained by modulating a dither piezo with one of the R9plus low voltage outputs. A  $\pm 15$  V DC power output is used to power a custom amplifier to detect the oscillation amplitude of the quartz tuning fork.

Optical signal information is sent to the R9plus from the Princeton Instruments Lightfield software through a LabView interface developed in our group. The optical signal in a user-defined spectral window is integrated and sent to a DAQ card (Measurement Computing DT3016) which transduces the signal to an analog voltage that is read by the R9plus. In this way, optical images can be correlated with topographic information in the R9plus software with fast acquisition speeds of  $<50$  ms/pixel.

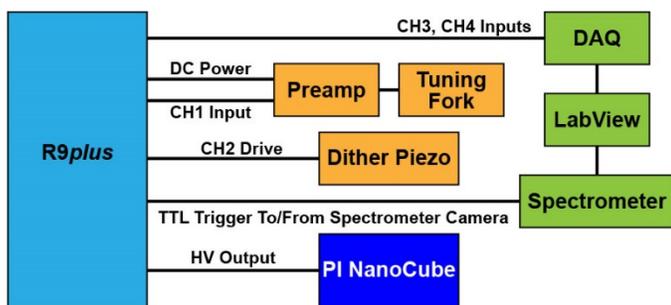


Figure 1. Wiring schematic of positioners, shear force feedback hardware, and optical signal hardware with the R9plus.

## Experimental Setup

A schematic of the TEPL spectroscopy setup is shown in Figure 2a. For the experiments, the sample was mounted to the PI nanopositioner with sub-nm

precision positioning below an electrically driven and controlled quartz tuning fork (32 kHz resonance frequency), which was used to regulate the tip-sample distance using the AFM shear-force amplitude feedback. Electrochemically etched Au tips (5–10 nm apex radius) were attached to the tuning fork and coarsely positioned using a piezoelectric stepper motor. In the TEPL spectroscopy setup, the sample was mounted at a  $35^\circ$  angle to the tip axis to maximize the electric field confinement. Excitation was provided by a helium-neon laser beam (632.8 nm,  $<1$  mW) with a half wave plate for polarization control that was focused onto the tip-sample interface using an objective lens. Photoluminescence signal was collected in a backscattering geometry, passed through a dichroic mirror with a 633 nm cut-off, and sent to a spectrometer (SpectraPro 500i, Princeton Instruments) with a thermoelectrically cooled, electron-multiplied, charge-coupled device (CCD, ProEM+: 1600 eXcelon3, Princeton Instruments). The spectrometer was calibrated using a hydrogen mercury lamp and a 150 g/mm grating blazed for 800 nm is used to provide high bandwidth spectral information.

## Radiative Control of Dark Excitons

Excitons (Coulomb-bound electron-hole pairs) are elementary photoexcitations in semiconductors that can couple to light through radiative relaxation. In contrast, dark excitons show anti-parallel spin polarization with generally forbidden radiative emission (Figure 2b). Here we demonstrate a tip-enhanced nano-optical approach to observing dark excitons with out-of-plane transition dipole orientations at room-temperature in  $WSe_2$  with Purcell factor control through the tip-sample nanocavity (Figure 2c). With all previous approaches relying on cryogenic temperatures, this approach provides a new and facile way to harness excitonic

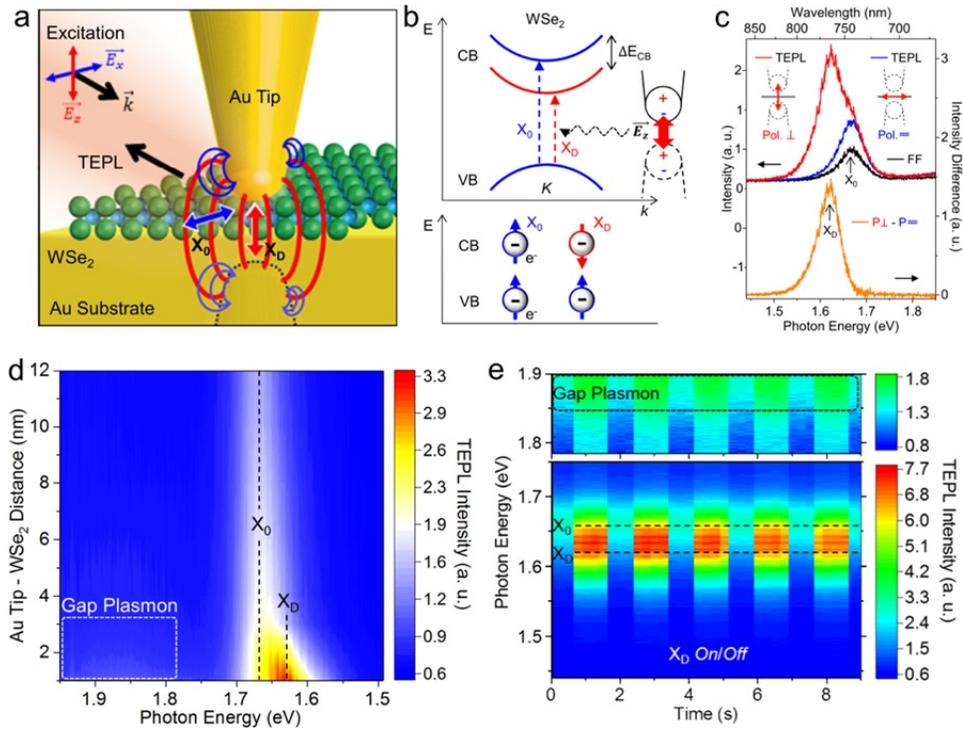


Figure 2. (a) Schematic of the TEPL spectroscopy setup. (b) Physical model of dark excitons. (c) Spectral signatures of dark excitons ( $X_D$ ) and bright excitons ( $X_0$ ). (d) Spectral evolution of dark exciton PL as a function of tip-sample distance exhibiting precise control by the R9plus. (e) Demonstration of controlled enhancement of the dark exciton signal by modulation of the AFM tip position.

properties in low-dimensional semiconductors for quantum optoelectronics and other applications.

In addition, this tip-enhanced nano-optical approach allows us to switch and programmatically modulate the dark exciton emission of a monolayer WSe<sub>2</sub> at room temperature for the first time. Using the plasmonic nano-cavity, we demonstrated a  $\sim 6 \times 10^5$ -fold enhancement in dark exciton photoluminescence quantum yield achieved through coupling of the antenna-tip to the dark exciton out-of-plane optical dipole moment, with large Purcell factor of  $2 \times 10^3$ . We then controlled this Purcell factor by precisely changing the tip-sample distance to decrease the near-field interaction (Figure 2d) and leveraged this technique to programmatically modulate the dark exciton signal by precisely controlling the tip-sample nano-cavity in time and space (Figure 2e).

These experiments demonstrate the ability to measure optical signals that are not accessible through room temperature far-field optical measurements and the ability to control these signals through precise tip-sample positioning.

### Why We Use RHK R9plus

Accessible, user-defined inputs allow for seamless integration of externally measured signals. This allows us to pre-characterize the sample by measuring the far-field optical signal to identify regions of interest on the sample before engaging in shear force feedback.

Optical signals can be easily correlated to topographic features due to R9plus' ability to obtain real-time imaging of multiple signal channels such as topography, TERS, SHG, TEPL, FWM, etc.

The *R9plus* software has an easy to use GUI interface which enables flexible region of interest selection (user defined XY pixel number) with features like drift correction and image referencing.

Numerous digital inputs and outputs are available to trigger external instruments required for our experiments (e.g. the spectrometer camera). This allows synchronized data collection between AFM signals and spectrometer data channels.

Setting up a Phase-Locked Loop (PLL) is not typically a simple task as there are feedback loops that need to be correctly tuned for proper function and to avoid a tip crash. However, the *R9plus* software not only makes it easy to find the resonance frequency of the tuning fork, but the built-in feedback tests used to properly adjust the feedback parameters of the PLL make the process of PLL setup extremely simple.

The *R9plus* also has a highly advanced “Lock Guard” capability that helps protect the probe from damage by continuously monitoring up to six data channels, retracting the probe within microseconds when detecting any out-of-bounds condition.

Our experimental design is constantly evolving. Since everything is controlled digitally, the *R9plus* allows us to easily reconfigure our setup. Often times, only simple modifications to the IHDL<sup>®</sup> file are required to define a new experimental design which minimizes the need to change external wiring.

## Future Implementations of *R9plus* Capabilities

There are many capabilities of the *R9plus* that have not been explored in this Application Note that we plan to implement in the future. One example is the implementation of the dual scan capability. We

currently use separate stages for both tip and sample but would like a better way to control these stages in a streamlined manner. With the dual scan capability and the numerous feedback loops available in the *R9plus*, we will be able to choose between scanning the sample stage (for larger range scans) and the tip (for smaller range, higher resolution scans) all within the user interface of the *R9plus* software.

An added benefit to the dual scan feature we foresee is the ability to quickly find the laser “hot spot” on the sample for optimal laser alignment. By scanning the tip position and monitoring optical feedback, the laser “hot spot” can be quickly located and the tip can be moved to a location within that “hot spot”.

Another feature we hope to explore further is the Q-control capability for tuning the quality factor (Q) of the tuning fork. Q-control is particularly useful since a large Q factor results in slower response times with amplitude feedback detection, leading to undesirable scanning times. Having Q-control eliminates this issue and allows measurements to be taken in a wide range of temperatures and in ultra-high vacuum conditions.

## Additional Information Related to This Work

Park, K.-D. et al. Radiative control of dark excitons at room temperature by nano-optical antenna-tip Purcell effect. *Nat. Nanotechnol.* 13, 59–63 (2018).

RHK Technology, Inc.  
1050 East Maple Road  
Troy, Michigan USA  
T: 248-577-5426 F: 248-577-5433  
[RHK-Tech.com](http://RHK-Tech.com)

© 2019 RHK Technology, Inc.  
All rights reserved.  
The information is subject to change  
without notice.